

INTERNATIONAL UNION OF PURE AND APPLIED CHEMISTRY

ANALYTICAL CHEMISTRY DIVISION
COMMISSION ON SPECTROCHEMICAL AND OTHER OPTICAL
PROCEDURES FOR ANALYSIS*

**Nomenclature, Symbols, Units and their Usage in Spectrochemical
Analysis – VII**

MOLECULAR ABSORPTION SPECTROSCOPY, ULTRAVIOLET AND VISIBLE (UV/VIS)

(Recommendations 1988)

Prepared for publication by

K. LAQUA¹, W. H. MELHUIH² and M. ZANDER³

¹Institute for Spectrochemistry, D-4600 Dortmund 1, FRG

²Institute of Nuclear Sciences, DSIR, Lower Hutt, New Zealand

³Rütgerswerke AG, Kekuléstrasse 30, D-4620 Castrop-Rauxel, FRG

*Membership of the Commission during the period (1979–1987) this report was prepared was as follows:

Chairman: J. Robin (France 1979–81); A. Strasheim (South Africa 1981–85); J. M. Mermet (France 1985–87); *Vice-Chairman:* K. Laqua (FRG 1983–85); *Secretary:* R. Jenkins (USA 1979–81); L. R. P. Butler (South Africa 1983–87); *Titular Members:* Yu. I. Belyaev (USSR 1979–81); K. Laqua (FRG 1979–83); W. H. Melhuish (New Zealand 1985–87); J. M. Mermet (France 1983–85); I. Rubeska (Czechoslovakia 1979–85); C. Sénémaud (France 1983–87); A. Strasheim (South Africa 1979–81); A. M. Ure (UK 1985–87); M. Zander (FRG 1985–87); *Associate Members:* C. Th. J. Alkemade (Netherlands 1979–85); L. R. P. Butler (South Africa 1979–83); H. Ebel (Austria 1981–85); Z. R. Grabowski (Poland 1979–83); G. M. Hieftje (USA 1983–87); G. F. Kirkbright (UK 1981–83); K. Laqua (FRG 1985–87); B. V. L'vov (USSR 1983–87); R. Manne (Norway 1981–85); W. H. Melhuish (New Zealand 1983–85); J. M. Mermet (France 1979–83); R. Müller (Switzerland 1979–81); N. S. Nogar (USA 1983–87); N. Omenetto (Italy 1979–87); E. Plsko (Czechoslovakia 1979–85); J. Robin (France 1981–85); R. O. Scott (UK 1979–81); C. Sénémaud (France 1979–83); R. Sturgeon (Canada 1985–87); A. M. Ure (UK 1981–85); J. P. Willis (South Africa 1985–87); M. Zander (FRG 1979–85); *National Representatives:* J. H. Cappacioli (Argentina 1981–85); A. J. Curtius (Brazil 1983–85); K. Danzer (GDR 1985–87); K. Zimmer (Hungary 1979–87); S. Shibata (Japan 1981–87); L. Pszonicki (Poland 1979–87); H. T. Delves (UK 1985–87).

Republication of this report is permitted without the need for formal IUPAC permission on condition that an acknowledgement, with full reference together with IUPAC copyright symbol (© 1988 IUPAC), is printed. Publication of a translation into another language is subject to the additional condition of prior approval from the relevant IUPAC National Adhering Organization.

Nomenclature, symbols, units and their usage in spectrochemical analysis – VII. Molecular absorption spectroscopy, ultraviolet and visible (UV/VIS) (Recommendations 1988)

This report is 7th in the series on Spectrochemical Methods of Analysis issued by IUPAC Commission V.4. It is concerned only with absorption spectra obtained by measuring the transmittance of light through a sample as a function of wavelength. Other techniques such as photoacoustic methods or reflectance measurements will be considered in later reports. The present report has four main sections (a) terms relating to absorption processes, (b) instrumental factors, (c) measuring techniques, and (d) factors influencing precision and accuracy.

Although absorption spectroscopy has been used for chemical analysis for well over 100 years, there are still many inconsistencies in terminology in the published literature. The American Chemical Society (ACS) has, in its journal Analytical Chemistry, suggested nomenclature for absorption spectroscopy for papers published by ACS. It should be noted that some IUPAC recommendations differ from these and furthermore include terms such as double-wavelength, difference and derivative spectroscopies which are not considered in the ACS report.

CONTENTS

1. Introduction
2. Fundamentals of molecular absorption spectroscopy (UV/VIS)
 - 2.1 The UV/VIS absorption spectrum
 - 2.2 The Beer-Lambert-Bouguer law
3. Instrumental factors
 - 3.1 Radiation sources
 - 3.2 Sample compartment
 - 3.2.1 Liquid samples
 - 3.2.2 Gaseous samples
 - 3.2.3 Solid samples
 - 3.2.4 Special cells
 - 3.3 Data acquisition and processing
4. Measuring techniques
 - 4.1 Qualitative analysis
 - 4.2 Quantitative analysis
 - 4.3 Spectral background correction
 - 4.4 Difference absorption spectroscopy
 - 4.5 Double-wavelength spectroscopy
 - 4.6 Derivative spectroscopy
 - 4.7 Absorbance matching
5. Factors influencing precision of absorbance measurements
 - 5.1 Random fluctuations
 - 5.2 Temperature effects
 - 5.3 Inhomogeneous samples
6. Factors influencing accuracy of absorbance measurements
 - 6.1 Spectrometric factors
 - 6.2 Wavelength accuracy

- 6.3 Spectral bandwidth
- 6.4 Stray radiation
- 6.5 Polarization
- 6.6 Optical beam effects
- 6.7 Scattering
- 6.8 Fluorescence effects
- 6.9 Cell factors
- 6.10 Sample stability
- 7. Factors other than instrumental that influence absorption spectra
- 8. Terms, symbols and units used in molecular absorption spectroscopy
- 9. Index of terms

1. INTRODUCTION

A series of documents dealing with nomenclature, symbols and units used in spectrochemical analysis is issued by IUPAC.

Part I (Pure Appl. Chem., 30, 653-679 (1972)) and Part II (Pure Appl. Chem., 45, 99-103 (1976)) are concerned mainly with general recommendations in the field of emission spectrochemical analysis.

Part III (Pure Appl. Chem., 45, 105-123 (1976)) deals with the nomenclature of analytical flame spectroscopy and associated procedures.

Part IV (Pure Appl. Chem., 52, 2541-2552 (1980)) concerns X-ray emission (and fluorescence) spectroscopy.

Part V (Pure Appl. Chem., 57, 1453-1490 (1985)) deals with the classification and description of radiation sources.

Part VI (Pure Appl. Chem., 56, 231-245 (1984)) covers molecular luminescence spectroscopy.

This document, Part VII, is concerned with molecular absorption spectroscopy (UV/VIS).

In the IUPAC Manual of Symbols and Terminology for Physicochemical Quantities and Units, 2nd revision (Pure Appl. Chem., 51, 1-41 (1979)) section 2.8 deals with quantities related to spectroscopy; see also IUPAC Manual "Quantities, Units and Symbols in Physical Chemistry" 1988 (publ. for IUPAC by Blackwell Scientific Publications, Oxford 1988) pp. 22-28.

Molecular absorption spectroscopy in the ultraviolet (UV) and visible (VIS) is concerned with the measured absorption of radiation in its passage through a gas, a liquid or a solid. The wavelength region generally used is from 190 to about 1000 nm, and the absorbing medium is at room temperature; however, in some cases measurements at temperatures above (e.g. in enzyme assays) or below room temperature may be advantageous or necessary. This document is restricted to the conventional means for measuring UV/VIS spectra i.e. transmission of radiation as a function of wavelength.

Not included in this document are terms relating to other methods for obtaining molecular spectra such as by measuring reflectance or by the variation of radiant power (e.g. fluorescence, phosphorescence) as a function of the excitation wavelength (*excitation spectrum*, see Part VI). Similarly the measurement of the heat generated in the vicinity of absorbing molecules as a result of the dissipation of excitation energy, which is a measure of the absorbed radiation, (*photo-acoustic spectroscopy*) is not included.

Although molecular absorption spectra are more meaningfully presented as a function of wavenumber (cm^{-1}), the more commonly used quantity is wavelength (nm) and this quantity will accordingly be used for this document. Where wavenumber is used in special cases, this will be indicated.

Many of the terms relating to instrumental factors in absorption spectroscopy are covered in Parts I, III and VI.

2. FUNDAMENTALS OF MOLECULAR ABSORPTION SPECTROSCOPY (UV/VIS)

2.1 The UV/VIS absorption spectrum

Molecules which absorb photons of energy corresponding to wavelengths in the range 190 nm to about 1000 nm exhibit UV/VIS absorption spectra. The quantized internal energy E_{int} of a molecule in its electronic ground or excited state can be approximated with sufficient accuracy for analytical purposes, by

$$E_{int} = E_{el} + E_{vib} + E_{rot} \quad (1)$$

where E_{el} is the electronic, E_{vib} the vibrational and E_{rot} the rotational energy, respectively. Absorption of a photon results in a change of the electronic energy accompanied by changes in the vibrational and rotational energies. Each vibronic transition, i.e. a particular electronic plus vibrational transition, corresponds to an absorption band consisting of rotational lines. In liquids and solids the rotational lines are broad and overlap so that no rotational structure is distinguishable.

The UV/VIS absorption spectrum of a molecular species is normally represented as a graph of some characteristic for the radiation absorbed as a function of wavelength. The graph is representative for that species, solvent, concentration and temperature. If a linear energy scale for the abscissa is preferred, then wavenumber, $\tilde{\nu}$ is used instead of wavelength, λ .

When the absorption of UV/VIS radiation by a solute is measured in a highly viscous or solid matrix at low temperature (less than about 100 K) a low temperature UV/VIS absorption spectrum results.

Highly structured spectra can be obtained when the UV/VIS absorption of a solute in certain polycrystalline matrices (e.g. n-alkanes, cycloalkanes, inert gases such as rare gases) is measured at low temperatures. For all spectra the solvent, solvent temperature and solute concentration should be specified (see Note a).

Direct recordings of these low temperature UV/VIS spectra are very useful for the identification of compounds; they are less useful in quantitative analysis because of the difficulty in measuring the true absorbance (see Section 2.2) of the sample, which usually exhibits high radiation scattering.

2.2 The Beer-Lambert-Bouguer law

The Beer-Lambert-Bouguer law, generally called the Beer-Lambert law, may be written for a single absorber either gaseous or in solution,

$$-\log_{10} (\Phi_t / \Phi_o) = -\log_{10} \tau_i = \epsilon c b = A \quad (2)$$

where Φ_t is the monochromatic radiant power transmitted by the absorbing medium, Φ_o is the monochromatic radiant power incident on the medium, τ_i is the internal transmittance ($= \Phi_t / \Phi_o$), ϵ is the molar (decadic) absorption coefficient, c is the amount concentration, b the absorption path length and A the (decadic) absorbance. These terms and their preferred units have already been defined in Parts I, III, and VI (Table 4).

Internal transmittance τ_i , i.e. transmittance of the medium itself, disregarding boundary effects, has to be distinguished from the total transmittance τ . The difference, which is mainly due to reflection losses associated with cell windows, can be compensated by using matched cells (see Section 3.2.1).

Absorptance (or absorption factor) α is defined by $\alpha = 1 - \tau$ where reflection is assumed to be negligible.

The Beer-Lambert law holds only if the absorbing species behave independently of each other, and if the absorption occurs in a uniform medium. Further, the incident radiation must be parallel, monochromatic (see Note b) and there should be no measurable saturation effect due to depletion of the ground state molecules. Causes for deviations from the Beer-Lambert law are listed in Section 7.

Note a. Terms such as Shpol'skii or quasi-linear spectra should not be used.

Note b. In practice parallel, monochromatic radiation is not always used. Convergence or divergence of the light beam as found in practice, will cause only minor deviations from the Beer-Lambert law. Section 6.3 discusses errors due to non-monochromatic radiation.

3. INSTRUMENTAL FACTORS

An instrument for measuring molecular absorption spectra (UV/VIS) usually consists of a radiation source, an optical system including a spectral apparatus, a sample compartment, a radiation detector and a system for data acquisition and data processing. Means for amplitude modulation and/or wavelength modulation may also be part of the instrument.

The classification of instruments according to single beam or double beam operation, recording, non-recording etc. is covered in Part IX, which also contains definitions and nomenclature on optical systems relevant to molecular absorption spectroscopy. Radiation detectors and modulators are treated in Parts VI and XI. Part V (radiation sources) does not deal with sources used in molecular spectroscopy. These will be covered in this section.

3.1 Radiation sources (see Note a)

Pertinent factors relating to the properties of continuum radiation sources are

the spectral distribution defined as the variation of the spectral radiance L_λ , with wavelength,
 the maximum spectral radiance, $L_\lambda(\text{max})$ within the usable wavelength range,
 the wavelength at this maximum, λ_{max} ,
 the usable wavelength range, defined by the lower limit λ_l and the upper limit λ_u at which the spectral radiance is a specified fraction of $L_\lambda(\text{max})$.

Continuum sources are normally used for molecular absorption measurements, whereas spectral-line sources (see Part V) are employed for wavelength calibration of a spectrometer. Examples of continuum sources commonly used are

tungsten-halogen lamps, which have a radiance temperature (see Part V) T_r of ≈ 3000 K and therefore have maximum spectral radiance at a wavelength^r of about 1.2 μm ; they are widely used in the visible and near ultraviolet spectral region (above 330 nm),
 deuterium lamps (gas-discharge lamps) which emit strongly in the UV region below 330 nm; the continuous spectrum has deuterium atomic emission lines superimposed on it,
 xenon arc lamps which give a continuum from below 190 nm to above 1000 nm.

Examples of spectral-line sources are

low-pressure mercury-discharge lamps, which are sometimes used for measuring absorbances at fixed wavelengths. Such lamps are also useful for wavelength calibration,
 Tunable lasers with and without frequency doubling and/or Raman shifting are high intensity sources with narrow spectral bandwidths. Their use may enable the spectral apparatus to be omitted. They may be either continuous (cw) or pulsed in nature.

3.2 Sample compartment

3.2.1 Liquid samples. Liquid samples are usually contained in sample cells which are placed in sample cell holders. Cell holders may be heated or cooled in order to control the temperature of the liquid in the sample cell.

The important characteristics of sample cells are,

cell shape (e.g. rectangular, cylindrical),
 absorption path length, b , defined as the length of the radiation path through the absorbing medium; it is equal to the cell path length, l , in the case of single-pass cells at normal incidence of radiation,
 volume and cross section,
 window material (window thickness and degree of deviation from parallelism of the windows are also important).

A pair of cells with closely similar optical properties are called matched cells. One cell is the sample cell while the other, the reference (or blank) cell contains the solvent or a reference solution (see Section 4.4). In double beam spectrometers, radiation is passed either simultaneously or alternately through the cells. In single beam instruments the cells are moved sequentially into the radiation beam.

Note a. Radiative properties of sources should not be described by photometric units (e.g. candela m^{-2}) (see Part I).

3.2.2 Gaseous samples. Gases and vapours are measured in gas cells similar to those used for liquids. Generally the cell pathlength is much greater. Gases at any pressure are contained in *closed cells* for measurement.

3.2.3 Solid samples. Solid samples are held in *solid-sample holders*. When solid samples are measured, difficulties may be experienced e.g. in matching the sample and reference pathlengths.

3.2.4 Special cells. *Low temperature cells* are required for certain applications. These may include *cooled cells*, *thermally insulated cells*, and *cold-finger cells*.

A *stopped-flow cell* comprises a small-volume absorption cell connected to a rapid mixing chamber.

A *multiple-pass cell* is constructed in such a way that mirrors either form part of the cell or are mounted in the sample cell holder. It permits multiple passage of radiation to increase the absorption pathlength.

A *continuous-flow cell* allow the liquids (or gaseous) sample to pass through the cell continuously while absorption measurements are made.

A *variable pathlength cell* is a cell whose pathlength can be varied either continuously or in steps by means of spacers.

3.3 Data acquisition and data processing

The equipment used for data acquisition and data processing can be classified according to the form of the information required. In the simplest case the output may present the transmittance or absorbance in an analogue or digital form. Further processing of the output signal enables various functions of the original signal to be obtained. These include

- absorbance
- log absorbance
- averaged spectra (with enhanced signal-to-noise ratio)
- derivative spectra (see Section 4.6)
- with additional processing, background correction (see Section 4.3)

For the fast acquisition of data, a *polychromator* (see Part III) fitted with a detector that enables spatial resolution, e.g. a *vidicon tube* or *silicon photodiode array*, together with a multichannel analyser may be used. The whole detection system is called an *optical multichannel analyser*.

4. MEASURING TECHNIQUES

The sample type and the information required determine which of the various techniques available will be used when conducting a molecular absorption analysis. The following are some of the more important methods.

4.1 Qualitative analysis

The identification of an analyte may be achieved by comparing the absorption spectrum of the unknown substance with graphs or tables of the spectra of known substances. In some cases two or more analytes may be recognized.

4.2 Quantitative analysis

A known analyte can be determined by measuring the absorbance at one or more wavelengths and using the Beer-Lambert law and the molar absorption coefficient to calculate its amount concentration. If the concentration is expressed in other units (e.g. g/L) the corresponding *specific (decadic) absorption coefficient* has to be used. Concentrations can also be determined from an *analytical function* or *analytical calibration curve* where the latter is obtained by plotting the measured absorbance of different *reference solutions* (or gases or solids) against their known concentrations. A graph of absorbance against concentration is a straight line passing through the origin if the Beer-Lambert law applies (see Section 7 for causes of deviations).

Multicomponent analysis of a mixture consisting of n absorbing analytes is possible provided the Beer-Lambert law holds, by measuring the absorbance at k suitable wavelengths with $k \geq n$. For each wavelength λ_a ($a = 1, 2 \dots k-1, k$) the total absorbance is given by

$$A(\lambda_a) = b \sum_{i=1}^n \epsilon_i(\lambda_a) c_i \quad (3)$$

where $\epsilon_i(\lambda_a)$ is the molar (decadic) absorption coefficient of analyte i at the wavelength λ_a and c_i its molar concentration. The ratio $A(\lambda_a)/b$ is called *linear (decadic) absorption coefficient*. This quantity is also called *linear absorbance*.

The concentrations of the n analytes may then be calculated from the k simultaneous equations.

4.3 Spectral background correction

The *spectral background absorbance* of a sample arising, for example, from the presence of an impurity with a weak, broad absorption band, can be subtracted from the analyte absorbance by graphical or algebraic methods when the spectral background absorbance is known. In practice, however, this applies only when the spectral background absorbance varies in a simple way (e.g. as a linear or quadratic function of wavelength; for other methods see Sections 4.5 and 4.6).

4.4 Difference absorption spectroscopy

A highly concentrated analyte in the analytical sample can be determined with better precision by replacing the blank (reference) cell by one containing a solution of the analyte or other absorber of known concentration (*difference absorption spectroscopy*). Difference spectra can also be obtained by computer or other subtraction methods.

4.5 Double-wavelength spectroscopy

The effect of spectral background due to impurities, solvent or radiation scattering may be reduced if the difference in the absorbances of a sample measured at two selected wavelengths is obtained. This is often achieved by repetitively switching from one wavelength to the other. *Double-wavelength spectroscopy* does this automatically by allowing two beams of radiation of different wavelength to pass through the cell. One beam is fixed at a longer wavelength and the other measures absorbance while being scanned over a limited wavelength range at shorter wavelengths.

4.6 Derivative spectroscopy

The *first (second, ...)* derivative absorption spectrum of a molecule is defined as first (second, ...) derivative, $dA(\tilde{\nu})/d\tilde{\nu}$, $(d^2A(\tilde{\nu})/d\tilde{\nu}^2, \dots)$ of the absorbance A as a function of wavenumber $\tilde{\nu}$. Wavelengths may be used in place of wavenumbers but the shape of the derivative spectra will be slightly different. When derivative spectra are obtained at low temperature, they are called *first (second, ...) derivative low temperature absorption spectra*, (specifying the solvent, temperature and solute concentration).

Derivative spectra are usually obtained by digital differentiation or by wavelength modulation of the radiation entering the sample cell. The *wavelength modulation interval* has to be much less than the bandwidth of any absorption band in the spectrum. The derivative spectrum in terms of wavenumber can be calculated from the spectrum in terms of wavelength by

$$dA(\tilde{\nu})/d\tilde{\nu} = (-\lambda^2) dA(\lambda)/d\lambda \quad (4)$$

$$d^2A(\tilde{\nu})/d\tilde{\nu}^2 = (\lambda^4)d^2A(\lambda)/d\lambda^2 + 2\lambda^3 dA(\lambda)/d\lambda \quad (5)$$

The use of derivative spectroscopy decreases the signal-to-noise-ratio. However, it can improve the detection of a sharp band in a broad background, or a narrow shoulder on a broad main band. Also gradual changes in spectral background or source flux will be less pronounced in derivative spectroscopy.

The first and second derivatives of the Beer-Lambert law are (assuming $d\Phi_0/d\tilde{\nu} \equiv 0$),

$$\frac{d\Phi_t/d\tilde{\nu}}{\Phi_t} = -2.303 c b \frac{d\epsilon}{d\tilde{\nu}} \quad (6)$$

$$\frac{d^2\Phi_t/d\tilde{\nu}^2}{\Phi_t} = [2.303 c b \frac{d\epsilon}{d\tilde{\nu}}]^2 - 2.303 c b \frac{d^2\epsilon}{d\tilde{\nu}^2} \quad (7)$$

Second derivative spectra are predominantly used in quantitative analysis.

The possible methods for the quantitative evaluation of derivative spectra are illustrated in Fig. 1 and are called *tangent* (Fig. 1a), *peak-peak* (Fig. 1b) and *peak-zero* (Fig. 1c) methods.

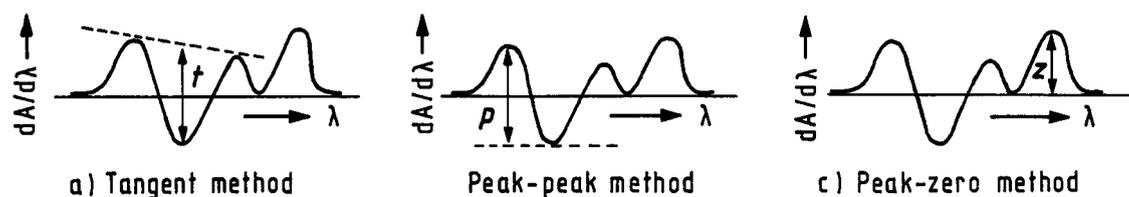


FIG. 1 : Quantitative evaluation of first derivative spectra, the quantitative measure being t in FIG. 1a), p in b), z in c)

4.7 Absorbance matching

Absorbance matching is a procedure where the concentration of a known analyte may be determined by diluting the sample with solvent until the absorbance matches the absorbance of a known concentration of the analyte in the reference cell. This method is particularly useful if the Beer-Lambert law does not hold.

5. FACTORS INFLUENCING PRECISION OF ABSORBANCE MEASUREMENTS

5.1 Random fluctuations

Random errors limit the precision of analysis (see Part II). When measuring very large or very small absorbances, uncertainties due to *random fluctuations* become particularly large. To obtain better precision in the absorption measurement it is necessary to adjust the sample concentration or cell pathlength to bring the absorbance into the range 0.1 to 1.0. The theoretical minimum error occurs at a *best precision absorbance* of about 0.43 for a spectrometer with a detector which is thermal noise limited, e.g. phototube or photodiode; and of about 0.86 for a spectrometer with a detector which is shot noise limited, e.g. photomultiplier.

5.2 Temperature effects

Temperature variations will to a greater or lesser extent affect all instrument functions. The absorbance of the sample, as well as the sample factors considered in section 6.7, may also depend on temperature. All of these effects give rise to *temperature errors*.

5.3 Inhomogenous samples

Errors due to inhomogenous distribution of absorbing species in the analytical sample are called *inhomogeneity errors*. They may be observed by probing the sample volume with an incident beam of radiation of reduced cross-section.

6. FACTORS INFLUENCING ACCURACY OF ABSORBANCE MEASUREMENTS

Accuracy, discussed in this section, refers to systematic errors which introduce bias in the measurement. Additional measurements must be made before errors such as those specified below can be detected and corrected.

6.1 Spectrometric factors

Any deviation from linearity of the response of the detector to the measured radiant power may cause a *non-linearity error*.

If insufficient time is allowed for the reading to settle or if an absorption peak is scanned too rapidly a *settling error* results.

If the two beams in a double-beam spectrometer are not fully equivalent in transmitted power nor are corrected to be so, a *base-line error* occurs, e.g. due to unmatched cells.

6.2 Wavelength accuracy

If there is a difference between the (mean) wavelength of the radiation entering the sample cell and the indicated wavelength on the spectrometer scale, an error in absorbance may occur. This error is called a *wavelength error*.

6.3 Spectral bandwidth

To measure the true shape, particularly the true maximum of an absorption band, the spectral bandwidth $\Delta\lambda$ of the instrument (see Part I) must be much less than the width of the absorption band. A *spectral bandwidth error* results from using too large a bandwidth relative to the absorption band being measured.

6.4 Stray radiation

A spectrometer set to pass radiation of a particular wavelength band always has a small amount of *stray radiation* of other wavelengths. Since the sample may absorb more (or less) of this stray radiation than of the radiation at the selected wavelength an error can occur. This error is called *stray radiation error*.

6.5 Polarization (for definitions see Part IX)

The radiation leaving the monochromator will rarely be completely unpolarized. *Polarization errors* may arise from the fact that the absorbance of a sample (especially a solid) could depend on the polarization of the incident radiation and from the polarization dependent response of the photodetector.

6.6 Optical beam effects

For wavelength-scanning spectrometers, an error may be introduced if the image position on the photodetector changes. Reflection of the incident radiation, e.g. between the cell walls, is another source of error and results in a measured absorbance slightly higher than the true absorbance. These errors are collectively termed *optical-beam errors*.

6.7 Scattering

The presence of particulate matter, emulsions, micelles, etc. may cause radiation scattering. This will result in further attenuation of the transmitted beam and the measured absorbance will be too high. This error is called the *scattering error*.

6.8 Fluorescence effects

Some samples are excited to fluoresce by the incident radiation beam. Added to the transmitted radiation beam, the fluorescence results in an erroneous reading, called the *fluorescence error*. It is particularly noticeable if the photodetector is situated close to the sample.

6.9 Cell factors

An error in the measured absorbance of a sample can occur if the incident beam does not fall perpendicularly to the windows of the cell, or if the cell windows are contaminated or have some other imperfection. These factors result in *cell errors*.

6.10 Sample stability

The absorbance of some samples may change with time, e.g. as a result of photochemical reaction, formation of aggregates or adsorption on the cell wall. Errors due to these changes are called *sample errors* (see Section 7).

7. FACTORS OTHER THAN INSTRUMENTAL THAT INFLUENCE ABSORPTION SPECTRA

The main factors that may affect the absorption spectrum and often result in deviations from the Beer-Lambert law are listed in Table 1. These alterations in the spectrum may appear either as a *wavelength shift* with little change in band shape, or as major alterations in band shape and position. Often more than one of the factors listed below are relevant as causes for changes in absorption spectra.

TABLE 1. Factors other than instrumental that influence absorption spectra

Factor	Cause	Information	Process*
(1) concentration	self-association	association equilibrium constant	$nA \rightleftharpoons A_n \quad (n \geq 2)$
(2) pH	acid/base (protolytic) equilibrium	protonation equilibrium constant	$A + H_3O^+ \rightleftharpoons AH^+ + H_2O$
(3) time	thermal chemical reaction (including solvolysis)	rates of reaction	$A \rightarrow B$
(4) (radiant) power	photochemical reaction	rates of reaction	$A \xrightarrow{h\nu} B$
	photochromism	equilibrium constant and reaction rates	$A \rightleftharpoons B$
(5) presence of component B	complex formation	equilibrium constant	$A + B \rightleftharpoons AB$
(6) temperature	thermochromism	equilibrium constant	$A \rightleftharpoons B$
(7) solvent	solute-solvent interactions	transition type	

* A and B are reacting species

8. TERMS, SYMBOLS AND UNITS USED IN MOLECULAR ABSORPTION SPECTROSCOPY

Term	Symbol	Practical Unit	Notes
radiant energy	Q	J	see Parts I and II
radiant power	$\Phi = dQ/dt$	W	see Part I
radiant intensity	I	$W\ sr^{-1}$	see Parts I and II
spectral radiance	$L_{\lambda}(B_{\lambda})$	$W\ m^{-2}\ sr^{-1}\ nm^{-1}$	
radiant power incident on absorbing medium	Φ_o	W	
radiant power transmitted by absorbing medium	Φ_t	W	
radiant power reflected by sample	Φ_r	W	
radiant power absorbed by medium	Φ_a	W	
transmittance or transmission factor	τ	1	$= \Phi_t/\Phi_o$
reflectance or reflection factor	ρ	1	$= \Phi_r/\Phi_o$
absorptance or absorption factor	α	1	$= 1 - \tau$
internal transmittance	τ_i	1	
internal absorptance	α_i	1	
(decadic) internal absorbance	A	1	$= -\log_{10} \tau_i$
linear (decadic) absorption coefficient	a, K	cm^{-1}	$= A/b$
molar (decadic) absorption coefficient	ϵ	$L\ mol^{-1}\ cm^{-1}$	$= A/(c\ b)$
specific (decadic) absorption coefficient	d	$L\ g^{-1}\ cm^{-1}$	
molar concentration of absorber	c	$mol\ L^{-1}$	
wavelength	λ	nm	
wavenumber	$\tilde{\nu}$	cm^{-1}	$= 1/\lambda$
spectral bandwidth of spectrometer	$\Delta\lambda$	nm	see Part I
wavelength modulation interval	$\Delta\lambda_{mod.}$	nm	wavenumber may also be used
absorption pathlength	b	cm	
cell pathlength	l	cm	

9. INDEX OF TERMS

absorbance (Section 2.2)
 absorptance (Section 2.2)
 absorption band (Section 2.1)
 absorption factor (Section 2.2)
 absorption pathlength (Section 3.2.1)
 absorbance matching (Section 4.7)
 amount concentration (Section 2.2)
 amplitude modulation (Section 3)
 analytical calibration curve (Section 4.2)
 analytical function (Section 4.2)
 averaged spectra (Section 3.3)

base line error (Section 6.1)
Beer-Lambert law (Section 2.2)
Beer-Lambert-Bouguer law (Section 2.2)
best precision absorbance (Section 5.1)
blank cell (Section 3.2.1)

cell error (Section 6.9)
cell pathlength (Section 3.2.1)
closed cell (Section 3.2.2)
cold-finger cell (Section 3.2.4)
continuous-flow cell (Section 3.2.4)
continuum source (Section 3.1)
cooled cell (Section 3.2.4)

data acquisition (Section 3)
data processing (Section 3)
derivative spectra (Section 3.3)
deuterium lamp (Section 3.1)
difference absorption spectroscopy (Section 4.4)
double wavelength spectroscopy (Section 4.5)

excitation spectrum (Section 1)

first (second ...) derivative absorption spectrum (Section 4.6)
first (second ...) low temperature derivative absorption spectrum (Section 4.6)
fluorescence error (Section 6.8)

inhomogeneity error (Section 5.3)
internal energy (Section 2.1)
internal transmittance (Section 2.2)

linear (decadic) absorption coefficient (Section 4.2)
linear absorbance (Section 4.2)
low-pressure mercury-discharge lamp (Section 3.1)
low temperature cell (Section 3.2.4)
low temperature UV/VIS absorption spectrum (Section 2.1)

matched cells (Section 3.2.1)
maximum spectral radiance (Section 3.1)
molar (decadic) absorption coefficient (Section 2.2)
multicomponent analysis (Section 4.2)
multiple-pass cell (Section 3.2.4)

non-linearity error (Section 6.1)

optical beam error (Section 6.6)
optical multichannel analyzer (Section 3.3)

peak-peak method (Section 4.6)
peak-zero method (Section 4.6)
photoacoustic spectroscopy (Section 1)
polarization error (Section 6.5)
polychromator (Section 3.3)
polycrystalline matrix (Section 2.1)

radiation detector (Section 3)
radiation source (Section 3)
random error (Section 5.1)
random fluctuation (Section 5.1)
reference cell (Section 3.2.1)
reference solution (Section 4.2)

sample cell (Section 3.2.1)
sample cell holder (Section 3.2.1)
sample compartment (Section 3)
sample error (Section 6.10)
saturation effect (Section 2.2)
scattering error (Section 6.7)
settling error (Section 6.1)
silicon photodiode array (Section 3.3)
solid-sample holder (Section 3.2.3)
specific (decadic) absorption coefficient (Section 4.2)

spectral apparatus (Section 3)
spectral background absorbance (Section 4.3)
spectral bandwidth error (Section 6.3)
spectral distribution (Section 3.1)
spectral line source (Section 3.1)
spectral radiance (Section 3.1)
stopped-flow cell (Section 3.2.4)
stray radiation (Section 6.4)
stray-radiation error (Section 6.4)

tangent method (Section 4.6)
temperature error (Section 5.2)
thermally insulated cell (Section 3.2.4)
total transmittance (Section 2.2)
tunable laser (Section 3.1)
tungsten-halogen lamp (Section 3.1)

usable wavelength-range (Section 3.1)
UV/VIS absorption spectrum (Section 2.1)

variable pathlength cell (Section 3.2.4)
vibronic transition (Section 2.1)
vidicon tube (Section 3.3)

wavelength error (Section 6.2)
wavelength modulation (Section 3)
wavelength modulation interval (Section 4.6)
wavelength shift (Section 7)

Xenon arc lamp (Section 3.1)